


HOW TO BUILD AN ELECTRONIC WITNESS WELL FOR RADIONICS

Mastering Radionics Series™

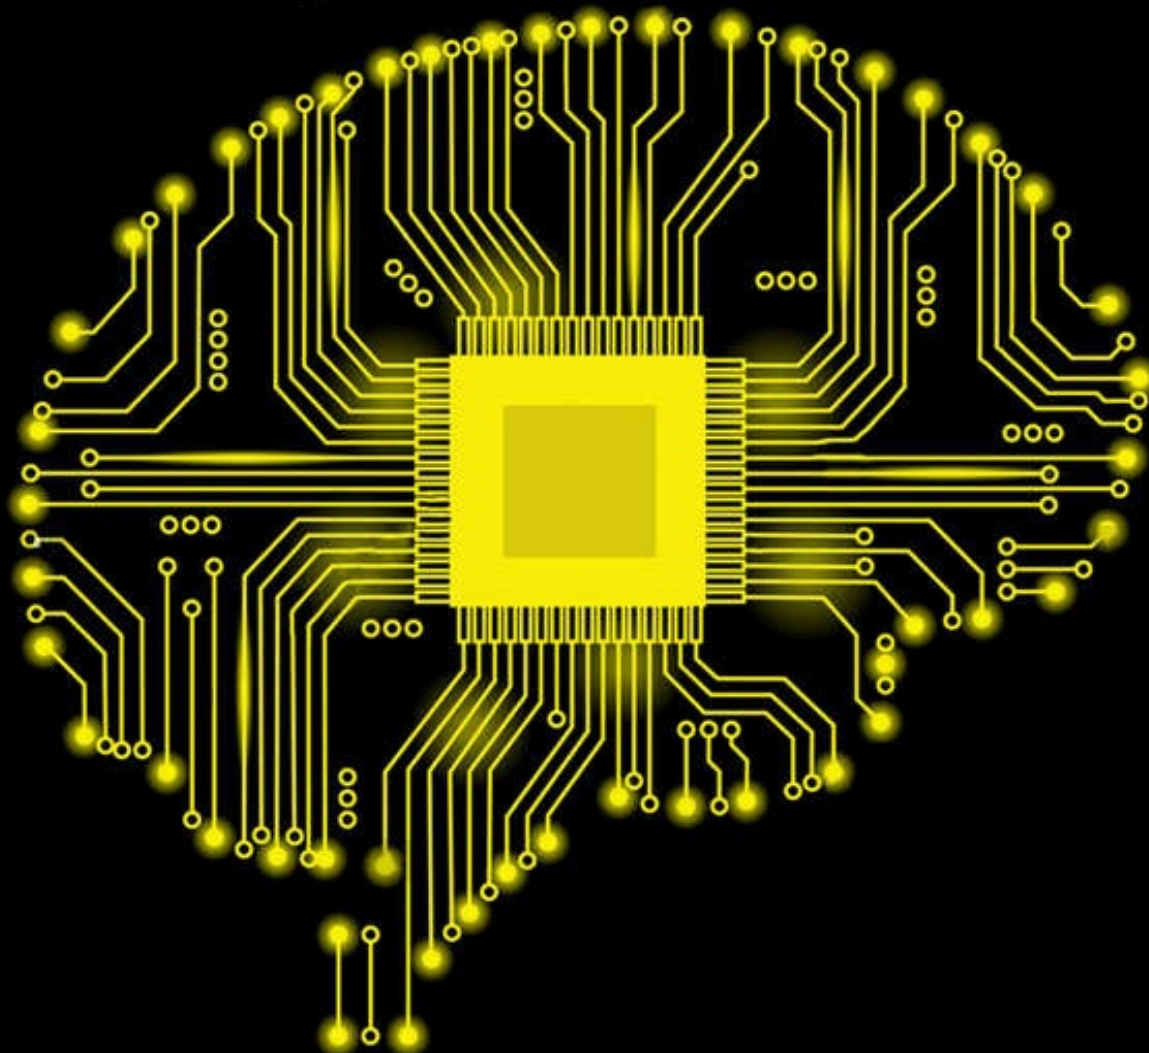

PETER V. RADATTI

How to Build an Electronic Witness Well for Radionics (E-Well)

Mastering Radionics Series TM

by Peter V. Radatti

April 2017



Table Of Contents

Inside Cover	
Table of Contents	
1 Preface and Dedication	
2 Copyright, ISBN and Legal Notices	
Disclaimer	
3 How to build an E-Well	

Parts List

Thumb Drives

- Picture Formats and Sizes
- Sample Form for Composite Witness
- 4 How to use and suggested usage
 - What Results Can You Expect
- 5 Rates used for the E-Well program
 - Unlock-1 (erase) Gem Stones
 - Lock Type 1 Gem Stones
 - Hell Burner 1.0
 - Hell Burner 2.0
 - ROSP Version 1.0
 - Vampire Repellent
 - Soul Integration Repair Protocol
 - KRT Psychic Attack Page 1
 - KRT Psychic Attack Page 2
 - Sacred Geometry Shapes and their Rates
- 6 Contact the Author and other books by the Author
- 7 Other Resources
 - Kelly Research Technologies
 - All Saints Church Ministry
 - Twisted Sage
 - Amazon.com UXCEL 6.7" X 3.1" Blue Metal Box
 - Amazon.com USB 3.0 A-Male to A-Female cable
 - Amazon.com CESS Terminal Binding Posts
 - Amazon.com Banana Plug Cords
 - Conshohocken Radionics
 - Dan Tuck's Thea Lamp
- 8 Bonus Material – Raspberry-Pi Computer
 - Inside End Page

Chapter 1 - Preface and Dedication

Preface

Radionics is fun. There is always some new problem to investigate and some new radionics program or device to invent or discover! This small booklet is intended to teach how to build an electronic witness well for use with KRT and other radionics machines. There are some really interesting things you can do with a well of this type, the most interesting are radionics programs that can be transmitted to a target 24-hours/day. Consider programs that provide spiritual protection, spiritual repair, blessings and enhanced luck. Consider a bubble of protection that reforms instantly upon breaking. Think about blessings such as Kiss of God (35.5-21.4) or the Ho'Oponopono Prayer (51.75-97 & 14-12.25 & 82.75-39) being received 24-hours per day! What would be the value of constant spiritual strengthening such as Soul Integration Repair or Spiritual Vampire Repellent? Basically, anything that can not be over balanced can be considered for broadcast.

An E-Well can not be used for everything, in fact there is a lot you can not do with it, and it is not a way to shotgun a problem but it is a subtle method of great potential which adds a new tool to our already vast tool box of Radionics.

This book assumes that you already understand radionics and have, at a minimal, read the book, "A Fun Course in Beginning Radionics Third Edition: Miracles in the palms of your hands" by the same author. That book is available on www.amazon.com . Search for the author's name of Radatti to locate easily.

This book is not intended as a substitute for the medical advice of physicians. The reader should regularly consult a physician in matters relating to his/her health and, in particular, with respect to any symptoms that may require diagnosis or medical attention. If you think you may be suffering from any medical condition, you should seek immediate medical attention. You should never delay seeking medical advice, disregard medical advice, or discontinue medical treatment because of information in this book.

Peter V. Radatti
April 2017

Dedication

This book is dedicated to my parents, Marie D. Radatti and Vincent J. Radatti, and to my Aunts and Uncles and friends. These people made me who I am. To the divine spirit who made all possible, including the miracle of life. *Additional Thanks to My Patron Saints:* Saint Jude Thaddeus, Mother Mary, Saint Rita. Finally, this book is dedicated to you my readers. May the knowledge contained herein help you to avoid some of the pain I experienced due to it's inaccessibility.

Chapter 2 – Copyright, ISBN and Legal Notices

Copyright Notice and Editions

Copyright © By Peter V. Radatti April 2017. All rights reserved.

All rights reserved under United States law and International law, including, but not limited to, the Berne Convention. This work is not in the public domain.

ISBN-13: 978-1545124819

ISBN-10: 1545124817

"How to Build an Electronic Witness Well for Radionics" is the second book in the "Mastering Radionics Series" of books. "Mastering Radionics Series" is a trademark of Peter V. Radatti.

The first book in this series is:

A Fun Course in Beginning Radionics Third Edition: Miracles in the palms of your hands. ISBN-13: 978-1542419970, ISBN-10: 1542419972

DISCLAIMER

This book is being presented to the reader for informational purposes only. It is meant to assist the general public in learning about the spiritual art known as Radionics. Nothing in this book is intended to serve as legal, medical, scientific, or spiritual advice in *any* matter; it is for educational purposes *only*. Each reader will and must draw their own unique conclusions about the material presented in this book, and if the reader attempts to implement said material, that is entirely their responsibility.

The information provided in this book is designed to provide helpful information on the subjects discussed. It is *not* meant to be used, nor *should* it be used, to diagnose or treat any medical condition; this is the sole purview of your physician. The publisher and author are not responsible for any specific health or allergy needs that may require medical supervision and are not liable for any damages or negative consequences from any treatment, action, application, or preparation to any person reading or following the information in this book. References are provided for informational purposes only and do *not* constitute endorsement of any websites or other sources. Readers should be aware that the websites listed in this book may change.

This book is not intended as a substitute for the medical advice of physicians. The reader should regularly consult a physician in matters relating to his/her health and, in particular, with respect to any symptoms that may require diagnosis or medical attention. If you think you may be suffering from any medical condition, you should seek immediate medical attention. You should never delay seeking medical advice, disregard medical advice, or discontinue medical treatment because of information in this book.

Without prejudice to the generality of the foregoing paragraph, we do not represent, warrant, undertake or guarantee:

that the information in the book is correct, accurate, complete or non-misleading;

that the use of the guidance in the book will lead to any particular outcome or result; or in particular, that by using the guidance in the book you will have any

result, or in particular, that by using the guidance in the book you will have any result.

If a section of this disclaimer is determined by any court or other competent authority to be unlawful and/or unenforceable, the other sections of this disclaimer continue in effect. If any unlawful and/or unenforceable section would be lawful or enforceable if part of it were deleted, that part will be deemed to be deleted, and the rest of the section will continue in effect.

Nothing in this paper should be considered medical advice. For the treatment of any medical condition you must seek the advice of a trained medical doctor.

Chapter 3 – How to Build an E-Well

The concept of an electronic witness well came from several different people. The first was from an article in the KRT Newsletter written by Ed Kelly. (<http://www.kellyresearchtech.com/>) This article spoke about different types of witnesses and their effectiveness. Another article was written by me and was on composite witnesses or how to create a witness when you could not get a photo, blood or hair sample. Finally, various radionics operators spoke about how they treat many animals or plants at the same time using a witness of many targets or many witnesses of multiple targets. Many of these discussions were held at the annual All Saints Radionics Masters Conference in Rapid City, SD.

There are many different ways of developing an electronic witness well. The simplest electronic witness well is to put witnesses on flash memory such as a thumb-drive and drop the memory in the radionics machine's witness well. Make sure you dowse to insure the witness is effective. I present a more complex and I believe more powerful E-Well here. This is the unit that I built and am using. Please modify the design to suite your needs.

Why an electronic witness well? Basically, I have several machines, some of which are dedicated to providing balancing 24-hours/day, 7-days/week for one target. This is wasteful so a method where a common radionics program could be sent to thousands of targets at the same time using only one machine would free up resources. This is not really unusual. I have seen operators using large witness wells with hundreds of photos as the target.

One method that I used and still use to broadcast without using an expensive radionics machine is an inexpensive primitive radionics machine called a Radionics Power Pod (RPP). While primitive, they work. There are no dials, so an RPP can only be used with preprogrammed crystals. To build your own RPP place a dual spin coil such as the Kelly Betar antenna in a tensor ring. You can buy tensor rings from both of these companies: <http://twisteddsage.com/> and <http://www.dtlightworks.com/> . The RPP works but is not as powerful as an actual powered and operating radionics machine.

Building an E-Well is simple and incorporates a RPP as part of the design. The parts list, in no order, is:

1. Steel cabinet or box

- 2. High quality USB thumb-drive (AKA: Jump Drive, Flash Drive. Plastic, not metal.)
- 3. 20 AWG copper magnet wire. Magnet wire is just copper wire that is coated in thin lacquer instead of plastic installation. This wire is what is used to create the electromagnet in transformers and other devices.
- 4. Kelly Dual Spin Betar Coil
- 5. Tensor ring

6. Banana plug jacks

- 7. A small piece of wood or plastic that fits on the floor of the cabinet
- 8. A USB extension cable

9. Hot Glue

- 10. Crazy Glue

11. Sand or crushed gem stones for programming

- 12. Container for the sand.
- 13. Banana plug cables to connect the E-Well to a radionics machine.

Using hot glue attach the Radionics Power Pod (Betar coil and Tensor ring) to the piece of wood. See picture below. I purchased a piece of scrap ¼-inch plywood at the hardware store for \$0.75. Underlayment (a type of very thin plywood) or a piece of plastic will work well. At the worse, cut the plastic lid from a coffee or other can to fit the bottom of the cabinet. Leave the KRT Betar coil in the protective plastic box it comes in. It will be sealed by the hot glue.



Open the steel cabinet and glue the wood base with the power pod to the bottom of the cabinet. It is actually important that you use a steel cabinet. Alternating layers of iron and carbon make an orgone accumulator. Steel is iron and wood or plastic is carbon. A single layer of iron and carbon is a weak but generating orgone accumulator. Never use aluminum. Aluminum and carbon creates a negative orgone accumulator also known as a DOR (Dead Orgone) accumulator. In addition to being an orgone accumulator I want to insulate the Radionics Power Pod from conductivity with the steel base. The wood/plastic block does this well.



Purchase a very high quality USB thumb-drive (AKA Jump Drive, Flash Drive). This is of critical importance. Inexpensive or novelty thumb-drives have a high rate of bit-rot. This means that the witnesses will degrade over time. I have personal experience with bit-rot and it is aggravating. At this time USB 3.0

capable drives are normally of high quality since the higher speed requires that better quality components are used. Fast USB ports are called USB 3.1 (Gen 2). (There are even faster versions but they require newer computers.) If you can find one of these it will use the high quality memory. Notice in the photo below it specifies USB 3.0. This is not a 3.1 device but is still high quality.

Basically, purchase a name brand, buy the highest speed that will work with your computer and do not buy cheap. You will notice in the photo below that I paid \$10.99 for the Toshiba drive. At the same store, a low quality USB 2.0 drive of the same size sold for \$7.99 and a low quality USB 3.0 drive of the same size sold for \$9.99. I paid only \$1 more but got high quality. Purchase only plastic drives. Do not purchase a metal drive. At the time I purchased my drive, Toshiba and Samsung made good drives. If you are unsure consult an expert.



How many radionics operators does it take to change a light bulb? Answer, none. They just balance the bulb until it works again. - Pete Radatti

Radionics: The art of smile and dial. - Unknown


Did you hear about the radionics razor blade? The company went out of business, they were only able to sell one to a customer. - Pete Radatti

Using the copper magnet wire, carefully wind it around the working part of the thumb-drive. Do not cover any of the USB plug. Make sure it is as tight to the


drive as possible. The wire should also be as close to each coil as possible but small mistakes are fine. See the photo below. No specific number of turns are required as long as the drive body is covered. Leave long tails on the wire and using sand paper or a knife remove the lacquer from the ends of the tails.



Drill two holes in the front plate of the cabinet large enough to fit the banana plug jacks. Mount the jacks into the holes and tighten the locking nuts in place. Attach the tails of the coil that you sanded from the thumb-drive to the wire lock downs on the inside of the banana plug jacks.

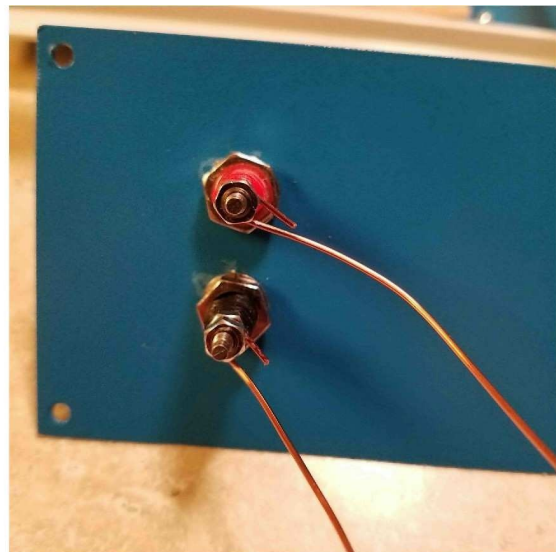

This is what the assembly looks like once you are done:

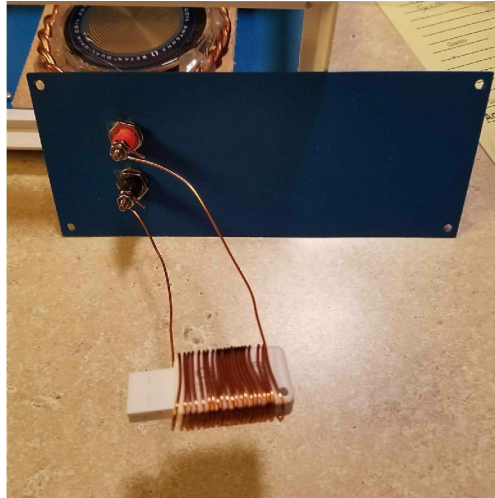

Reattach the front of the cabinet to the cabinet and bend the wire tails so the thumb-drive is centered over the Betar Coil. Here is a picture of the assembly before the tails are bent into place. You can also wait for this step until after you are done gluing inside of the cabinet. It is all a matter of how comfortable you are with tools.



Next fill a container with sand or crushed semi-precious gem stones. I prefer quartz crystal sand however crushed gem stones are the gold standard that have been proven by the test of time. Gem stones never lose their programming. Notice that the box is mostly filled and that all of the bottom is covered. It is not necessary or easy to completely fill the box. As long as the bottom of the box is always covered you have enough sand. I used one of the boxes a KRT Betar Coil

came in. Since sand is so small and fluid I seal the box using crazy glue. That is not as simple as it sounds. Measure out the sand in the box then pout it into a cup. Wash the plastic box out and thoroughly dry. This will remove static buildup. Quickly pour the sand into the center of the box and close the lid. It should close easily. Once closed hold it sideways and check there is enough sand. Then using a tube of crazy glue seal the place where the lid and the bottom of the box meets. This will keep the sand from coming out. You can also use hot glue but that tends to be messy.




Once the box is sealed program it in your Radionics machine. Use the potentizer well. Use the supplied programs in the back of this book. Unlock the sand. Since it has never been locked this clear it. Program in the ROSP Version 1 program followed by the Hell Burner Version 1 program. Once done, lock the sand using the supplied lock program. These rates will protect the entire system including the E-Well and the radionics system. At the same time these rates will be broadcast to the witnesses 24-hours/day 7-days/week even when turned off.

Don't worry about making changes in the future. You can unlock and change the programs in the sand/gems without removal from the E-Well.

Using a hot glue gun attach the box with the sand/gems to the top of the Radionics Power Pod. Only glue it in three spots but use a large amount. This is so if you ever want to change the program medium you can use a knife to cut the glue and remove the box.



You can also program the sand/gems after the system has been assembled. If you ever want to change the programs in the sand, take the lid off of the cabinet and put the entire E-Well inside of a large pottinger well. You can now unlock and add programs or clear the sand and reprogram. Don't forget to lock again when done. (Make a backup copy of the thumb-drive before you do this.)

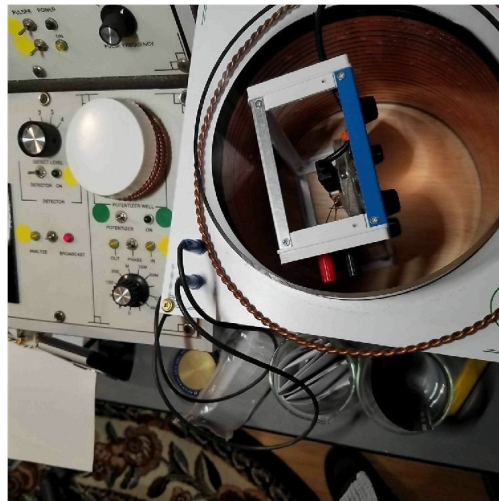


Position the thumb-drive with cable on the top and center of the sand box. Glue the thumb-drive and coil to the top of the sand box. Only glue it on the sides so you can use a knife to cut the drive away if you ever decide to upgrade the drive. Make sure the cable is attached to the thumb-drive before gluing or you may have a problem attaching it after the glue hardens. Buy a few small tie-wraps. In the photo below (left) the tie-wrap is orange in color. Also buy a few tie-wrap tie-downs. In the picture below it is the white plastic square with the perforated disk on top. The tie-wrap goes through the tie-wrap tie-down. The tie-down has double sided tape on the back. Attach it someplace logical in the box and tie the


USB cable down to it using the tie-wrap. (Photo right) This provides strain relief to the thumb-drive. (The strain relief may not be needed depending upon the cabinet strain relief device.)



Drill a hole in the back of the cabinet large enough to fit the USB extension cable though. Connect the cable to the thumb-drive. Attach a strain relief to the cable so it doesn't move the drive when the cable is used. There are many different types of strain relief, choose one that will work for you.

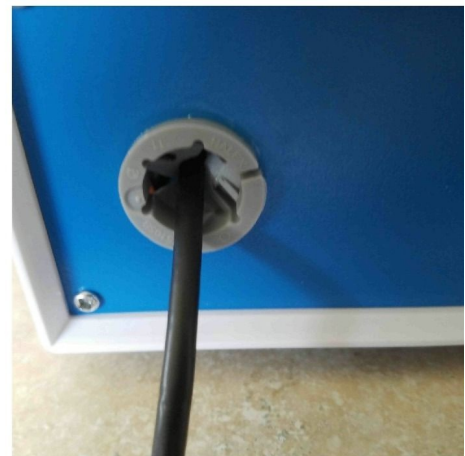

Close the cabinet and attach the banana plug cables. Photo left is a package of banana cables. Photo right is the E-Well with the cables attached to the front and to the INPUT jacks of a KRT Ag Workstation.

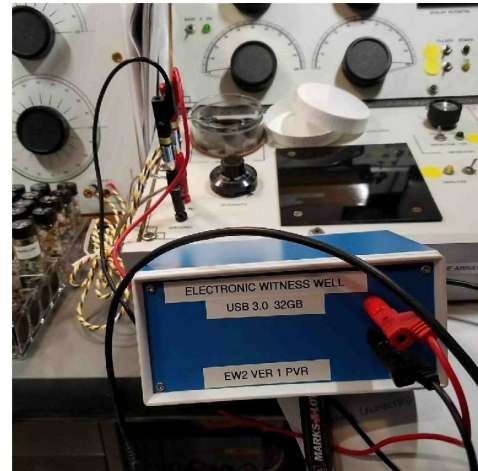

Attach a label to the front of the cabinet to make it look nice!



You are now ready to program the witness well with digital witnesses. Any photograph of a target that is at least 5 megapixels or higher will work. You may also want to enter a document with the photograph that further enhances the witness. (Composite witness) Basically any file format will work as long as you dowse for effectiveness first. Put the file sample on a thumb-drive and enter it in the witness well. Then dowse for a yes/no answer to the question, "Will this witness be effective enough to work for my intended purposes both now and in the future?". If you get a Yes then proceed. If you get a NO then you need to add information until you get to a YES. Examples of information is name, address, *etc.* Anything that clearly identifies the target and only that target.

A 5 megapixel photo is 2580 X 2048 pixels. This is actually 5.28 Megapixels. Picture file formats at this size will take up the following size in storage:

UNCOMPRESSED FORMATS

TIFF Monochrome 8bit/pixel	5.28 MB
RAW/DNG 10 bits/pixel	6.60 MB
RAW/DNG 12 bits/pixel	7.93 MB
RAW/DNG 14 bits/pixel	9.25 MB
RAW/DNG 16 bits/pixel	10.6 MB
BMP RGB 3x8 bit/pixel	15.9 MB
TIFF CMYK 4x8 bit/pixel	21.1 MB

COMPRESSED FORMATS

JPG 100% 24 bit/pixel	1.08 MB
JPG 90% 24 bit/pixel	539 KB
GIF 8 bit/pixel, 255 colors	1.60 MB
PNG lossless 24 bit/pixel	3.07 MB
Lossless JPEG	7.93 MB

If we assume the TIFF format at 21.1 MB and a 32GB thumb-drive which is 32,000 MB then 32,000 divided by 21.1 MB/photo is a bit over 1,516 photos per drive. If we add a composite witnesses and assume a small text file with every photo you should easily fit over 1,250 witnesses in the well. That means you can balance 1,250 targets at the same time using a single high quality radionics machine like a KRT personal workstation. If we assume the more common 24bit JPG format at 1.08MB each we can fit 29629 photos. Leaving lots of space for a composite witness you could store more than double the number of witnesses or about 2,500.

Since the number of witnesses that can be stored in the E-Well is very high there are precautions that you should take to protect your targets. One is to separate each target in the well. Use a separate directory for each witness. For example, lets says I want to put all of my pets into the well. I have Bebe the goat, Josie the pussycat ¹, Howard the dog and Bubbles the goldfish. I would create a directory of each of their names and put the witness or composite witness into the appropriate directory. While the witnesses are only separated by directory names

this separation is effective. There is no cross talk between witnesses. You may want to further organize these directories for ease of management. For example, I have each of these directories in my family directory. It makes it easy and fast for me to find things by organizing data in this way.

In general if you want to delete a witness from the E-Well you can overwrite it with a file of equal or larger size then delete it or you can use one of the super-delete programs available for purchase. This may or may not be important but always better to be safe than sorry. Generally when you delete a file from a computer it is not actually removed but just marked as deleted and the space made available for reuse. The data could last for a long time before being reused.

Here is a sample form that you can use to create a composite witness:

Name _____ Date. _____

Street Address _____


City _____ State _____ Zip Code _____

Phone # (if appropriate) _____

Date of Birth _____

Anything else that can help focus the target. Example, birthmarks, eye color, hair color, etc....



Connect the E-Well to the witness well input jacks on your system and you are ready to go.

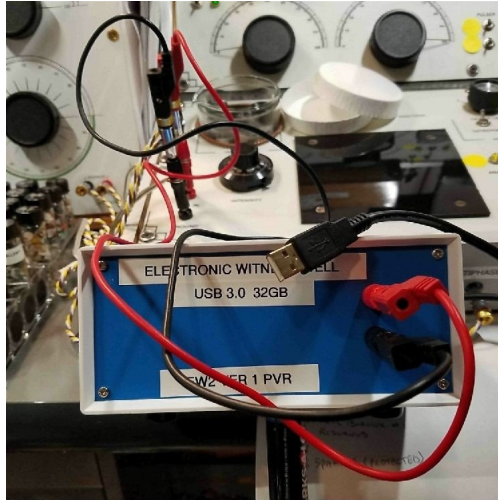

1 Insider joke for those that grew up watching the cartoon "Josie and the Pussycats"
[https://en.wikipedia.org/wiki/Josie_and_the_Pussycats_\(TV_series\)](https://en.wikipedia.org/wiki/Josie_and_the_Pussycats_(TV_series))

Chapter 4 - How to use and suggested usage

1. Put all of the witnesses you want on the device. Follow directions for separation of witnesses.
2. Connect the output banana plugs from the E-Well to the Input (Witness) jacks on your machine.

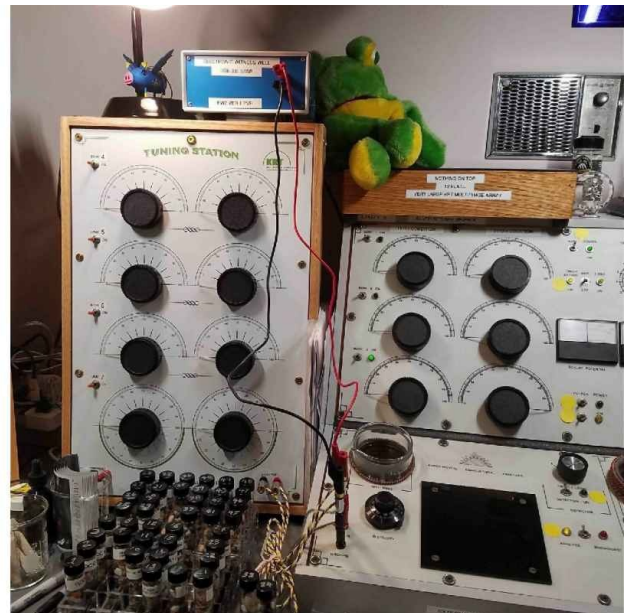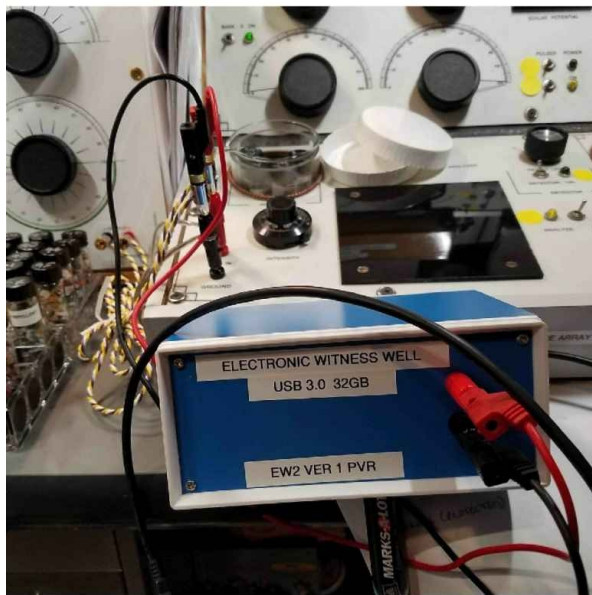

3. Determine what programs you want to broadcast and determine how long you want to broadcast. I strongly suggest you pick programs that can be broadcast 24-hours per day, 7-days per week. Things that can not be over broadcast are generally blessings and protections. Not all forms of protection are appropriate. Use stick and dowse for what can and can not be sent. Several of the programs that I developed can be sent in this way. An example is the Soul Integration Repair (SIR). It will have no effect if over broadcast but will repair any deviation as soon as it happens. The same can be said with bubbles of protection, they are safe. If a bubble is destroyed it is reformed. Blessings such as "Kiss of God" 35.5-21.4 can not be over broadcast. Many but not all, of the rates in VAMPIRE REPELLENT are good for this purpose. Be careful, keep your programs separated into tubes of sand for easy removal and check on everything

programs separated into tubes of sand for easy removal and check on everything often.

4. Put the programs you want to broadcast in the witness well. (tubes of sand/gems/crystals) If your witness well is not big enough I suggest the Large Witness Well sold by KRT. You can also combine programs by potentizing them one at a time into a new tube.

5. Potentizer OFF, Broadcast ON.

That is all there is to it. There is a slight difference between the rates sent by the Radionics Power Pod within the E-Well and what you broadcast via the radionics machine. If you want, and appropriate, you may rebroadcast these.

What results can you expect?

The simple answer is that I have no idea. Everyone reacts differently to balancing. In some cases people can feel the balancing as warmth or tingling. Most people can not.

The effect of 24 hour per day balancing is different than a single balancing and you will need to understand this difference and make allowances for it. In many ways, this is an advanced skill. Remember that some people have herxheimer reactions to balancing. A herxheimer reaction is a short term (days to weeks) detoxification reaction. Some of the following symptoms are common: flu-like symptoms, headache, joint and muscle pain, body aches, sore throat, general malaise, sweating, chills, nausea or other symptoms. ² Remember that what we are doing is spiritual and not medical in nature. Things happen based upon a spiritual basis, not a physical basis and are therefore hard to predict.

When the Conshohocken Radionics discussion club tested the E-Well for the first time the following results were noted: (Programs used are unpublished.)

Subject A: Burning stomach, constipation and excessive energy. Difficulty sleeping but no tiredness next day. Coffee consumption reduced from 3 cups to 1 cup. Burning faded in 2 days. General feeling of well being. Fading of some long term issues.

Subject B: Flu-like symptoms for 2 days. Felt more energetic.

Subject C: Did not notice anything.

Subject D: Excessive energy and difficulty sleeping but no tiredness. Pleased with new found energy.

Positive symptoms reported including more energy and happiness. Additional test subjects could not be contacted at time of publication. The longer the program runs the more positive symptoms are expected but again, only God knows.

Results will vary according to program used.

When selecting radionics programs to use, be careful in your selection. Use dowsing (stick) to determine if what you want to use is appropriate both now and during the life of the project. Use dowsing to determine if you should add someone to the well or if you need to do manual balancing prior to E-Well balancing. Follow all the rules that you would use if you were to balance a single witness in a machine for 24 hours per day.

Of course you don't have to use the E-Well 24 hours per day but that is it's most powerful use.

Chapter 5 - Rates used for the E-Well program

Unlock-1 (Erase) - gem stone rates (no password)

Run Unlock on gems or sand that is not locked and it clears them. Run Unlock once on gems or sand that IS LOCKED and it unlocks them without erasing. Of course run it twice and you unlock and clear/erase everything.

Unlock potentized Prayer Stones (gems) without changing the primary rates.	68.5-22.6 & 28.75-20.6 & 66.9-34 & 33.5-38.4 & 57-33.5 & 32-34.5
---	--

Lock-1 Gem Stones / Sand (no password)

This lock allows the frequencies to be copied but not modified, unless they are unlocked. No password is needed. The lock is not copied. Items locked in this way can be run through an airport x-ray machine without damage.

Maximize the potency of all frequencies. (Notes: Scan for appropriateness prior to use.) (All 6 banks are one frequency.)	28.25-31.75 &14-72.25 & 8.5-27.75 &12.5-50.25 & 49.25-42 &43.6-16.6
Lock and protect stones without password	&37.25-11.5

Hell Burner 1.0 (Use this one in well program)

Potentize gem stones or quartz sand with the ROSP program. Vampire Repellent, Psychic Attack and Sacred Geometry then lock it using Lock-1 Gem.

Hell Burner 2.0

Add in the SIR program.

ROSP Version 1.0

25-27.5	Prepare operator for maximum effectiveness in operating unit and results of operating unit with harm to no one.
27.75-38.75	Prepare unit for proper operation and maximum effectiveness of results with harm to no one.
38.5-58	Clear area of all bad and protect area during operation with harm to no one.
16.1-35 & 3.9-6.9	Install protective bubble of energy around system and operator that allows good energy to flow in and bad energy to flow out but does not allow bad energy in, with harm to no one.
12.00-22.00	White Light
35.5-21.4	Kiss of God.
29.75-6.1 & 2.9-2.5	Clear Witness Well of any impurities
23.9-24.75 & 31.9-11.9 & 9-0	Clear Potentizing Well of any impurities
32.6-33.6 & 16.5-12.9 & 20.25-21.5	Clear Stick Pad of any impurities
22.1-13.9 & 32-17 & 11.5-9.75	Ignore any impurities in Witness that may cause false values.

23.6-8.25 & 8.9-12.5	Enhance Stick for maximum effectiveness and correct answers
52.5-18.2 & 15-16 & 9-15 & 26.9-51.5	All rates entered on this system are modified to be "With Harm To No One".
19.75-11.5 & 37.4-17.5 & 17.75-23 & 31.1-21.25	Radionically Diagnose and Repair anything wrong with this unit.
67-27.5 & 31-35.9 & 14.2-27.7	Connect Radionics equipment to God.
59.9-65.5 & 63-50.75 & 89.9-72.5 & 32.9-45	Connect Radionics Operator to God.
60.5-59.5 & 34-49 & 49-24.1 & 42.5-40.6 & 40.5-33.5 & 43.2-54.5	Draw energy from God to power Radionics Operator.
64.5-49 & 33.9-57 & 33-65.4 & 48.5-73 & 37.8-41	Draw energy from God to power Radionics Device.
62-65.5 & 59.5-49.2 & 49-35.25 & 72.5-59.75 & 45-50 & 55.4-45.2	Seek divine protection from God during operation of Radionics device.
87.5-58.25 & 70.9-66 & 33.6-46.5 & 66.9-76	Do not allow Radionics Operator's personal life-force to be used in operation.
73-47.2 & 55.5-37 & 53.75-57.7 & 37.5-61.5	Do not allow false readings from minerals
86.5-29.75 & 26.1-38 & 20-56.2 & 52-66.75 & 60.4-52 & 69.9-71 & 75-79.75	Do not allow false readings from environmental issues.
44.9-17 & 11-15.5	Do not allow false readings from energetic issues.

& 17-15 & 22.9-18.6
& 12.75-15 & 24-27.5

VAMPIRE REPELLENT

Start with spiritual first aid:

- | | | | |
|----|-----|--|------------|
| 1. | KRT | Cords, Release All Needed cords reestablish themselves, so this is house cleaning. | 39.5-25.5 |
| 2. | KRT | Affirmation, I am surrounded by a strong, white light, I am protected from harm. You will need this, but it is not complete protection from a vampire. | 18.5-38.25 |
| 3. | KRT | Divine Protection | 48-58 |
| 4. | KRT | Gem Obsidian, Deflect Negativity, protection, healing | 77.5-71.75 |
| 5. | KRT | Italian Alder, protected peace | 70-62 |

Start the process of spiritual healing:

- | | | | |
|----|-----|---|-----------------|
| 6. | PVR | Kiss of God | 35.5-21.4 |
| 7. | PVR | To stir the chi in the body. Vampire attacks can cause blocks. | 23-23.6 |
| 8. | PVR | Install protective bubble of energy around witness that allows good energy to flow in and bad energy to flow <i>out</i> but does not allow bad energy <i>in</i> , with harm to no one. This is not a total answer because the vampire is taking your good energy out. | 16.1-35,3.9-6.9 |

Prevent it from happening again:

- | | | | |
|----|-----|--|---|
| 9. | PVR | Install a very sharp, spinning, outer bubble of protection around other bubbles of protection that can cut any unwanted cords or attachment that are drawing energy from witness. Notice: This only eliminates | 77.5-66.6
& 10-13.25
& 21.5-26.25
& 36.5-20.6
& 20.5-45.8 |
|----|-----|--|---|

unwanted cords, so if you are in love with the vampire (common), you will need to decide what you are going to do. There are healthy cords that exchange energy, so you want those to reestablish themselves. This bubble is not 100% protection by itself.

- | | | | |
|-----|-----|---|--|
| 10. | PVR | Forcefully and continuously break any cords that draw unhealthy amounts of life-force energy. Notice: This is different from #9 in that acts as a circuit breaker. There are times you may want to give energy but not at the cost of your spiritual health. | 12.5-47
& 17.5-34.75it
& 69.25-50.4
& 31.75-35
& 39.5-63
& 64.5-82.6
& 38.5-59.4 |
| 11. | EAA | Ho'Oponopono Prayer | 51.75-97
& 14-12.25 &
82.75-39 |
| 12. | PVR | Become repugnant to vampires This is a difficult one to implement, therefore the large number of rates. In addition, this is not proof by itself. It will make the target repugnant in the same way that cooked liver and spinach is repugnant to some small children. Be when setting the rates. You may break up the rates into batches, but they are all one rate. If you break them up, rescan time for each batch. | 50-23.9 & 23-33
68.9-58.1 &
27.26-5.25
27.8-73.4 &
23.8-12
36.5-38.4 &
15.6-16.5
57.1-44.75 &
14.5-91.2
45.2-27.2 &
48.75-22.9 |

Reestablish proper and healthy connection to life-force:

- | | | | |
|-----|-----|---|-----------------|
| 13. | KRT | Angelic Support, Connect with divine guidance | 36.5-35.5 |
| 14. | KRT | Attunement with God | 21-37 |
| 15. | KRT | Affirmation, Worthy of and joyously receive | 26-28.5 & 25.5- |

and use continuously an abundance of God's loving 10.5

16. PVR Reattach to Universal Life-force / God. This rate is very useful for everything, not just Vampires. Everything in existence needs a connection to God. Ensure that the connection always exists. You can balance this rate. 98-71 & 35.5-22
20-5 & 3.25-22.5
50.8-98.25 & 65-54.4

Soul Integration Repair Protocol

(SIR)

THIS IS IMPORTANT! The Spirit creates the Astral Body. The Astral Body creates the Physical Body. There are a lot of steps involved, but we know that Information Transfer is a critical part of that process. To a certain extent, you can consider that the transfer method for information is a type of circuit. While not the entire process, this attempts to correct any damage to the transfer and control circuits of the Soul that build the Astral and Physical bodies. The Soul projects the Physical body; it does not occupy it. Explanation: Many people think that the physical body is like a jar, and it contains the soul. That is incorrect. The soul projects the physical body in much the same way that a movie projector projects an image. The physical body is just an extension of the soul, and a weak one at that. If you are attempting to balance these, you want as high an Intensity as possible, always much higher than GV. It is appropriate to put these rates in jewelry. In addition, check White Light and balance, if necessary, with Psychic Attack.

This is also one of the ways that demons and negative entities gain entrance to the Astral Body and the Physical Body. Repair of the damage at the entry points makes it very difficult for these entities to attack.

IMPORTANT NOTE: Any rate marked with an asterisk is an entry point for demons and negative entities. You must check, then triple check your settings. The rate needs to be checked often if psychic attack is suspected. The critical value of the RHD rate will be specified in each case. This rate must be exact. Since it is a critical rate, you should always check for appropriateness and harm to no one. Better safe than sorry. All potentization times will vary.

Soul-to-Astral

Soul-to-Astral Primary Information Circuit

This is 1 rate on 3 banks.

Potentize into gems for 6 minutes

61 4 21 5 2-

Potentize into gems for 6 minutes.

01.4-21.5 &
22.5-25.6 &
7.5-62.25

Soul-to-Astral Secondary Information Circuit

This is 1 rate on 4 banks.

Potentize into gems for 11 minutes.

38.9-9 &
58.75-78 &
66.75-17 &
17.5-28.4

Soul-to-Astral Third Information Circuit

This is 1 rate on 3 banks.

Potentize into gems for 37 minutes.

33.9-87.6 &
52-70.4 &
22-60.5

Soul-to-Astral Fourth Information Circuit

This is 2 rates on 5 banks. The first rate takes 2 banks. The second rate takes 3 banks. Potentize the first rate into gems for 14 minutes.

100-49.5 &
16-17.6

Potentize the second rate into gems for 21 minutes.

34.5-14.9 &
71.4-37.75 &
57.75-35.75

Soul-to-Astral Fifth Information Circuit

This is 3 rates on 11 banks.

Potentize the first rate into gems for 32 minutes.

30.5-88 &
97-90 &
16.5-15.5

Potentize the second rate into gems for 42 minutes.

90.25-62.7 &
56-59.25 &
97.75-76 &

16.5-23.9 &
28.75-98.9

Potentize the third rate into gems for 13 minutes.

28.75-99 &
14.5-18.75 &
15.1-17.5 &
13.25-17.25

Soul-to-Astral Sixth Information Circuit

This is 1 rate on 3 banks.

Potentize this rate into gems for 16 minutes.

39.5-33 &
11-13 &
37.75-39

Soul-to-Astral Seventh Information Circuit

This is 1 rate on 5 banks.

Potentize this rate into gems for 25 minutes.

82.4-30.75 &
13-52.25 &
12.5-38 &
20.25-12.75 &
27.8-12.4

Soul-to-Astral Eighth Information Circuit(CRITICAL RATE)

This is 2 rates on 6 banks. (CRITICAL RATE)

Potentize the first rate into gems for 9 minutes.

24-28.75 &
13.75-45.75 &
27.75-29 &
9-25

Potentize the second rate into gems for 5 minutes. IMPORTANT NOTE: This rate is one of the entry points for demons and negative entities. This rate needs to be checked often if psychic attack is suspect. The critical value is the RHD rate of 14.5 .

14.9-14.5 &
15.75-20.6

15./5-6.6

Soul-to-Astral Ninth Information Circuit

This is 3 rates on 4 banks. (CRITICAL RATE) 44-56.1 &
Potentize the first rate into gems for 13 minutes. 28.5-28

Potentize the second rate into gems for 10 minutes. 43.25-39.9

Potentize the third rate into gems for 7 minutes. IMPORTANT NOTE: This rate is also an entry point for demons and negative entities. This rate needs to be checked often if psychic attack is suspect. The critical value is the RHD rate of 12.5

38.4-12.5

Soul-to-Astral Tenth Information Circuit

This is 4 rates on 4 banks. (CRITICAL RATE) 78.1-30.25
Potentize the first rate into gems for 14 minutes.

Potentize the second rate into gems for 16 minutes. 74.25-39.9

Potentize the third rate into gems for 13 minutes. 24.25-26

Potentize the fourth rate into gems for 18 minutes. IMPORTANT NOTE: This rate is also an entry point for demons and negative entities. This rate needs to be checked often if psychic attack is suspect. The critical value is the RHD rate of 15.2 .

37.5-15.2

Astral to Physical

Astral To Physical Primary Information Circuit

This is 3 rates on 7 banks. (CRITICAL RATE) 53-38 &
Potentize the first rate into gems for 19minutes. 19.5-13.4

Potentize the second rate into gems for 15 minutes. 88-44.75 &
25-68.25

Potentize the third rate into gems for 6 minutes. **IMPORTANT NOTE: This rate is also an entry point for demons and negative entities. This rate needs to be checked often if psychic attack is suspect. The critical value is the RHD rate of 14.6**

34-14.6 &
34-18.25 &
19.5-35.25

Astral To Physical Secondary Information Circuit

This is 3 rates on 3 banks.

Potentize the first rate into gems for 4 minutes. 15.1-42

Potentize the second rate into gems for 11 minutes. 54.5-10.25

Potentize the third rate into gems for 20 minutes. 42-22.75

Astral To Physical Third Information Circuit

This is 3 rates on 3 banks.

Potentize the first rate into gems for 19 minutes. 49.25-31

Potentize the second rate into gems for 16 minutes. 43.5-35.75

Potentize the third rate into gems for 19 minutes. 22.75-31.5

Astral To Physical Fourth Information Circuit

This is 3 rates on 5 banks.

Potentize the first rate into gems for 17 minutes. 34.25-8.5 &
9.5-94 &
51.25-44.5

Potentize the second rate into gems for 17 minutes 97.5-38.25

Potentize the third rate into gems for 13 minutes. 24.4-38.6

Astral To Physical Fifth Information Circuit

This is 3 rates on 5 banks.

Potentize the first rate into gems for 9 minutes. 58.4-33.6 &
18-21 &
15.1-13

Potentize the second rate into gems for 11 minutes. This is an important rate (RHD) but it is unknown why.

41-27.9

Potentize the third rate into gems for 13 minutes. This is an important rate (RHD) but it is unknown why.

26.5-18.7

Astral To Physical Sixth Information Circuit

This is 2 rates on 4 banks.

Potentize the first rate into gems for 16 minutes. 46.75-38.4 &
35.5-26.75 &
25-19.75

Potentize the second rate into gems for 19 minutes. Time will vary. This is an important rate, especially the RHD value of 13.25, but it is unknown why.

25.7-13.25

Astral To Physical Seventh Information Circuit

This is 2 rates on 4 banks.

Potentize the first rate into gems for 8 minutes. 26.6-17.5 &
8.5-14

Potentize the second rate into gems for 11 minutes. 27.1-21.9 &
13.25-30.25

Astral To Physical Eighth Information Circuit

This is 2 rates on 3 banks.

Potentize the first rate into gems for 15 minutes. 70.4-66 &
17.5-45.5

Potentize the second rate into gems for 13 minutes. 35-36.75

Astral To Physical Ninth Information Circuit

This is 4 rates on 7 banks.

Potentize the first rate into gems for 20 minutes. 32.5-13.25 &
20-5.25

Potentize the second rate into gems for 22 minutes. 17.4-27.6
19-19.25

Potentize the third rate into gems for 29 minutes. This is an important rate, especially the RHD value of 7.5, but it is unknown why.

27.5-7.5 &
16.5-10.75

Potentize the forth rate into gems for 11 minutes. 31.25-15

Astral To Physical Tenth Information Circuit

This is 2 rates on 3 banks.

Potentize the first rate into gems for 28 minutes. 34-27.5 &
19-25.75

Potentize the second rate into gems for 23 minutes. 22-23

Soul-to-Astral-to-Physical Basic Structure

There is basic information that defines an Astral and Physical body. Without this basic information, an Astral body would not be an Astral body; it would be something else. If this information becomes damaged, then it must be repaired. These rates are for humans only. The Soul, also known as the Spirit, is. It exists in perpetuity. It cannot be truly damaged, but it *can* collect negative stuff that does not allow it to project properly. Think of this process as burying a light in dirt. It is still bright, but no one can see it under all the dirt. If the dross on your soul is severe enough, then you just wouldn't exist because you could not project the next level toward a physical body. Without a Soul, everything else is moot. The fact that you exist at this physical level is proof that your soul exists. To understand this, I draw upon the parallel Christian concept of original sin or the Buddhist concept of inherited karma. We will attempt to clean the Soul, but very gently. We cannot destroy or modify the Soul, but we don't want to add any dirt, either. The Soul projects the Astral Body. The Astral Body projects the Physical Body. The information flow is bi-directional! Your physical body is much more of a projection than a container.

Information that defines the basic structure of an Astral Body

This is 3 rates on 7 banks.

Potentize the first rate into gems for 10 minutes.	9.5-23.9 & 7-17
--	--------------------

Potentize the second rate into gems for 7 minutes.	22.5-10 & 4.5-9.4
--	----------------------

Potentize the third rate into gems for 10 minutes. This is an important rate, especially the RHD values of 18 and 14.4, but it is unknown why.

17.3-18 &
18.5-14.4 &
16.5-20.25

Information that defines the basic structure of a Physical Body

This is 1 rate on 5 banks.

Potentize this rate into gems for 29 minutes.	11.5-15.5 & 12 10 5 0
---	--------------------------

12-16.5 &
12.5-50 &
16.5-100 &
25.9-30.25

Removal of Information that Does Not Belong in/on the Soul

This is 1 rate on 4 banks

Potentize this rate into gems for 18 minutes.

37-29.1 &
16.5-21.9 &
14.5-37 &
43-37.5

Removal of Information that damages the transfer of information from the Soul to the Astral Body

This is 1 rate on 7 banks.

Potentize this rate into gems for 11 minutes.

68.4-46 &
26-24.1 &
19.5-30.5 &
20.3-22.25 &
74.5-34 &
31.1-25

Removal of Information that Does Not Belong in the Astral Body

This is 2 rates on 4 banks.

Potentize the first rate into gems for 14 minutes.

20.75-24.5 &
28.1-11

Potentize the second rate into gems for 7 minutes.

28.6-30.75 &
13.5-11

Removal of Information that damages the transfer of information

from the Astral to the Physical Body .

This is 5 rates on 7 banks.

Potentize the first rate into gems for 20 minutes.

44.5-12 &
19-15

Potentize the second rate into gems for 18 minutes.

39.5-16.5 &
25.9-85.4

Potentize the third rate into gems for 18 minutes. The RHD value of 24.75 and the 18 minutes are critical values but it is unknown why. Pay close attention to the value while potentizing.

16.9-24.75

Potentize the forth rate into gems for 8 minutes. The RHD value of 9.2 is critical but it is unknown why.

71.9-9.2

Potentize the fifth rate into gems for 18 minutes.

31-77.25



Psychic Attack

Name:		Sex:		Project Intent:			
Animal Type:		Age:					
Description	Left	Right	Left	Right	Reading	Reading	Reading
Yes/No	100.00-	0.00					
General Vitality	9.00-	49.00					
White Light	12.00-	22.00					
<p>Dark Forces - Associated with directed negative thinking or energy, typically the result of singular emotional bursts rather than a long term attack. These rates usually respond rapidly to balancing, though the stronger the emotional charge, the longer the time to balance. The intensity of White Light should be within 50 of General Vitality. The ratio of White Light to any Dark Forces energy should be 10:1. <i>Broadcast on rate to reduce any value above 50.</i></p>							
Dark Force, Negative Thinking, Influences	11.00-	21.00					
Dark Force, Negative Thinking, Influences	11.50-	25.00					
Dark Force, Negative Thinking, Influences	16.00-	1.00					
Dark Force, Negative Thinking, Influences	25.50-	0.50					
Dark Force, Negative Thinking, Emotion, Influences	30.00-	16.00					
Dark Psychic Forces	26.30-	28.50					
<p>Negative Energies - Associated with non-directed negatively charged energies, including vortices and ley lines generated by the planet. Other forms include old patterns of information bound to a location, as in the case of paranormal activity. <i>Broadcast on rate to reduce any value above 50.</i></p>							
Implant Receiving, Psychic Attack Accompanied by Dark Force or Negative Blocking Body	20.00-	37.00					
Interference from Multi-Dimensional, Psychic Attack	57.00-	63.50					
Emotional, Psychic Toxins	10.75-	35.75					
Emotional, Psychic Toxins	16.25-	27.50					
Emotional, Psychic Toxins	17.25-	45.50					
Emotional, Psychic Toxins	25.75-	26.25					
Emotional, Psychic Toxins	26.50-	16.00					
Emotional, Psychic Toxins	36.00-	28.00					
Emotional, Psychic Toxins	38.25-	28.25					
Emotional, Psychic Toxins	42.75-	27.75					
Emotional, Psychic Toxins	26.25-	38.25					
Emotional, Psychic Toxins	46.50-	28.25					
Emotional, Psychic Toxins	55.75-	16.00					
Emotional, Psychic Toxins	56.25-	17.50					
Psychic Numbness	33.50-	32.00					
<p>Killer Psychic Force Rates - These energies are both directed and of a much higher intensity than Dark Forces. They may be the result of extreme emotions, produced by the mentally unstable or the work of structured negativity, including curses, spells or voodoo. These energies may also be introduced by discarnate entities, and this should be taken into account in cases of alcoholism, drug habit (prescribed or recreational), recent emotional stress, and traumatic injury. <i>Broadcast on rate to reduce any value above 50. Expect longer than average broadcast times.</i></p>							
Killer Dark Psychic Force	10.25-	34.50					
Killer Dark Psychic Force	11.50-	46.50					
Killer Dark Psychic Force	21.00-	11.00					
Killer Dark Psychic Force	25.00-	21.50					
Killer Dark Psychic Force, Dark Force, Influences	25.50-	scan					
Killer Dark Psychic Force	26.25-	28.50					
Killer Dark Psychic Force, Thinking	39.50-	69.50					
Killer Dark Psychic Force	46.50-	scan					
Killer Dark Psychic Force, Unknown	39.00-	13.00					

This information compiled for *experimental agricultural research only* and is not intended for use with

humans. If medical or mental health care is needed, please visit a licensed professional.

Copyright 2012, Kelly Research Technologies, Inc.

2011-02

Copyright 2012, Kelly Research Technologies, Inc.

Sacred Geometry Shapes and their Rates

Platonic Solids					
Tetrahedron	57.25-27		>800		
Hexahedron	92-99		>800		
Octahedron	55-49.50		>800		
Dodecahedron	20.75-93		>800		
Icosahedron	44.75-79		>800		
Icositetrachoron	93.50-79.25		>800		
Icosahedron-Pentagonal-Dodecahedron	56-60.75	74-87.50	>800		
Phi (Golden Ratio)	88.50-85.25		>800		
Archimedean solids					
Cuboctahedron	34-37.25				
<u>Icosidodecahedron</u>	28.50-95.50				
<u>Rhombicubeoctahedron</u>	95.50-18.25				
<u>Rhombicosi dodecahedron</u>	54.50-29.50				
<u>Rhombi truncated Cuboctahedron</u>	6.25-90.25				
<u>Rhombi truncated Icosidodecahedron</u>	52.50-45				
<u>Snub Cube</u>	77.50-83.25				
<u>Snub Dodecahedron</u>	97-50				
<u>Truncated Cube</u>	47.25-63.25				
<u>Truncated Dodecahedron</u>	83-81				
<u>Truncated Icosahedron</u>	13-92				
<u>Truncated Octahedron</u>	54.50-51.50				
<u>Truncated Tetrahedron</u>	70.50-77.25				

Chapter 6 - Contact the Author

If you are going to send me spam or hate-mail, please don't. If you are going to explain to me how I am misguided, please don't. If you have questions about what I wrote or have helpful suggestions, feel free to write. If you just want a forum to discuss Radionics, welcome. Telling me to dunk my head in a bucket is not helpful. I tried and didn't care for it.

My email for the purpose of this book is: peter@tigerteam.com

If the address gets bombed, I will discontinue it. Then, you might be able to contact me via the Conshohocken Radionics meetup site:

<http://www.meetup.com/radionics/>

There is a support site for this book and Radionics in general. The site is not a public site and is by invitation only. You are invited. Questions will be answered by members who feel like it, not just me. Evaluate answers before accepting them. Members of the site may offer ROS programmed crystals/sand for sale. I have nothing to do with that but I do permit it. Caveat emptor, "buyer beware". In a few cases, I might write about how I like some program; that is an opinion. Any inappropriate actions, such as spamming the site, flaming, or insulting others, will result in the offending person being banned. There is no recourse. Be respectful, play nice, and others will be respectful and play nice with you.


<http://www.tigerteam.com/bbs>

Thank you for reading my book. I look forward to your questions and comments.

Chapter 7 – Other Resources

Kelly Research Technologies

There are fantastic training and rate books available free from KRT, who manufactures professional-quality radionics devices. They also sponsor classes. Their website is: <http://www.kellyresearchtech.com>

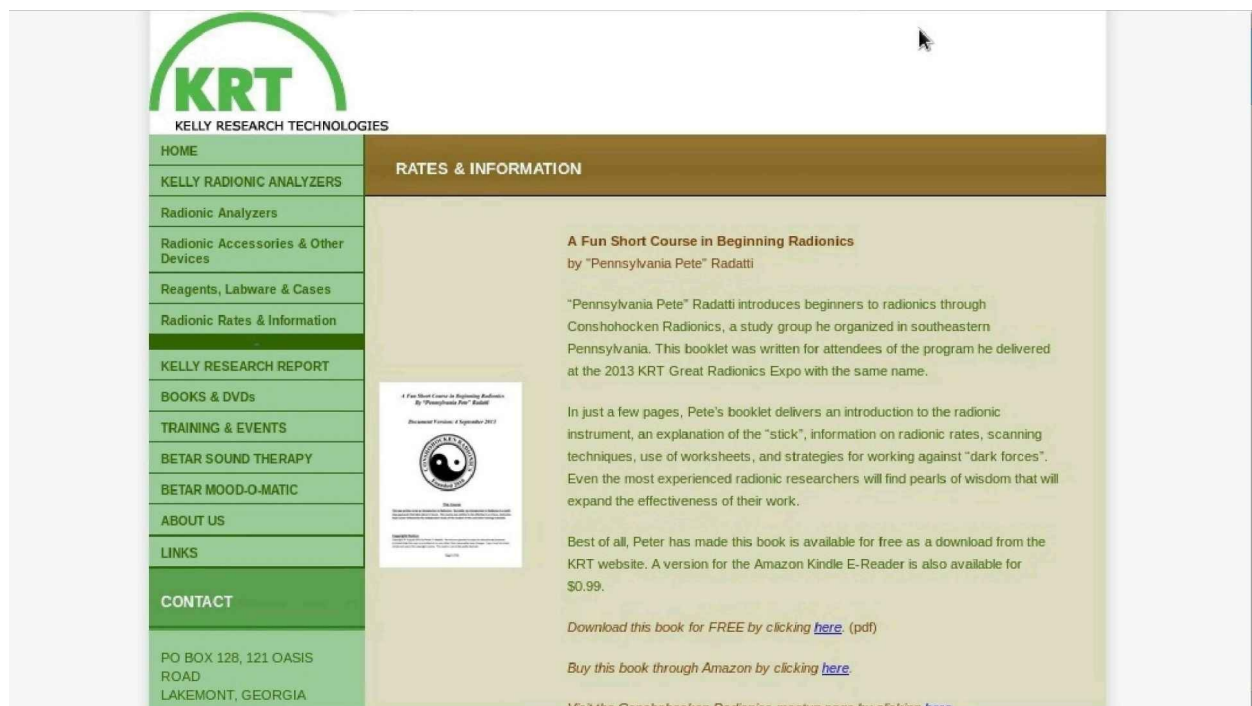

To download Ed Kelly's Radionics books, use the following link:

www.kellyresearchtech.com/download.html

Here are descriptions of the books from KRT's website:

"KRT Radionics Book 2: Applied Radionics


Take control of your energetic destiny with this hands-on manual featuring step-by-step instructions for safe and successful use of all KRT radionic analyzers and potentizers, as well as advanced strategies, techniques, and topics. Much of the information in this book is directly applicable to other two-dial analyzers, including Hieronymus, Rogers, Mattioda, and Lightning devices."

"KRT Radionics Book 3: Radionic Rates - Alpha


This book is the result of more than 35 years of compiling, collecting, and creating radionic rates for two-dial instruments. A reference volume for use in energetic research, this database includes more than 13,800 rates and is sorted alphabetically. Ideal for use with all Kelly instruments, as well as all Hieronymus, Rogers, Mattioda, Lightning, and SE-5 radionic devices."

All Saints Church Ministry . Wellness consultations and advanced training in energetics / metaphysics & radionics. For info call 605-787-5620 or email livingwordministrv8@yahoo.com

Twisted Sage – (www.twisted sage.com) Source of Tensor Rings

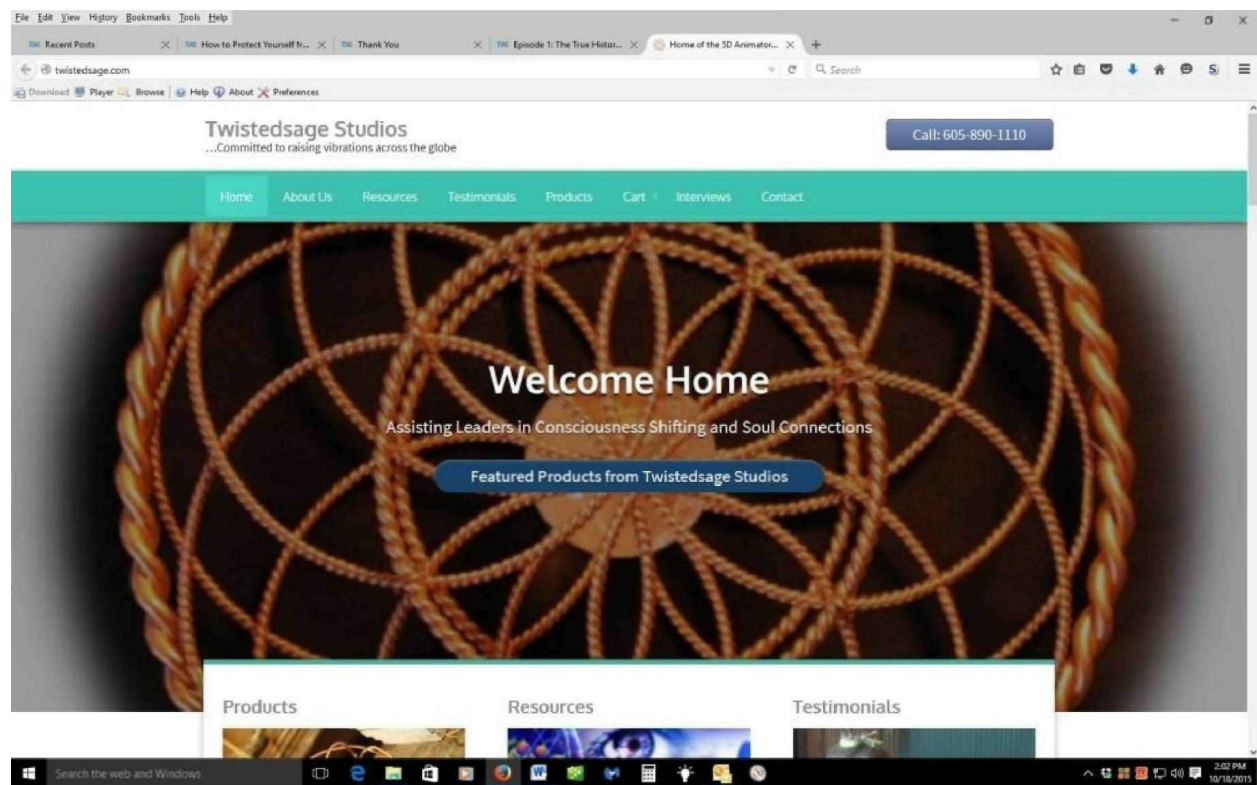

Amazon.com UXCEL 6.7" X 3.1" Blue Metal Enclosure Project Case DIY Junction Box \$21.29

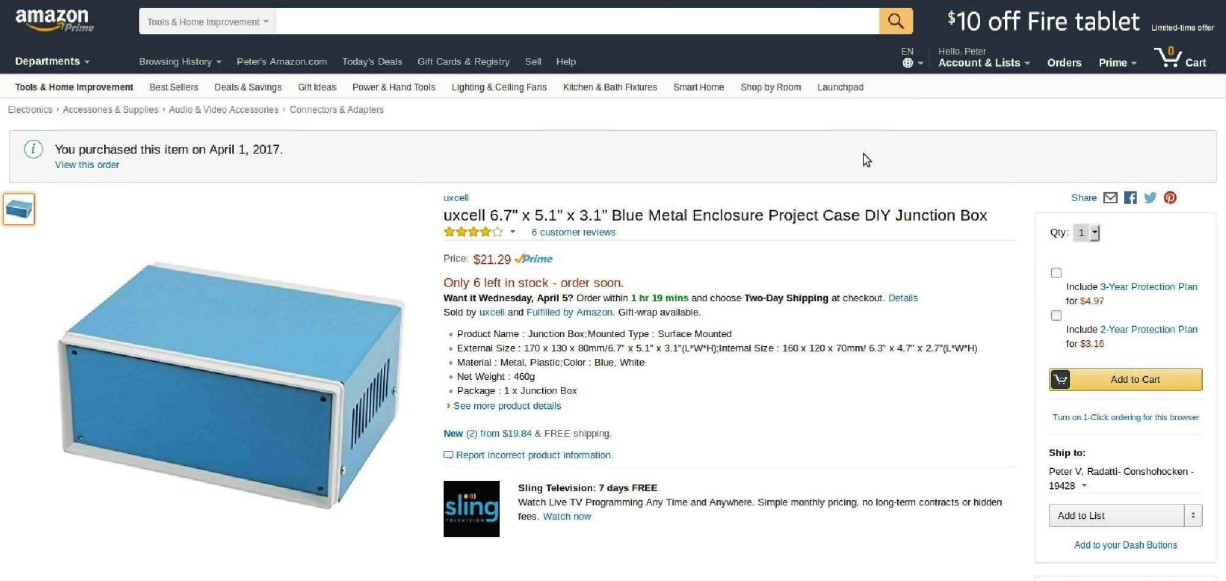

This screenshot shows the Amazon.com product page for the UXCEL 6.7" x 3.1" Blue Metal Enclosure Project Case DIY Junction Box. The page features a large image of the blue metal enclosure on the left. To the right, the product title is displayed in bold, followed by a star rating and the number of customer reviews. The price is listed as \$21.29, with a Prime logo indicating fast shipping. Below the price, there is a note about stock availability and a countdown timer for a Wednesday deal. The product details section lists specifications such as dimensions, material, and weight. On the right side of the page, there are options to add the item to the cart, a section for protection plans, and a shipping address field. The Amazon Prime logo and a search bar are visible at the top of the page.

amazon Prime

Tools & Home Improvement

Departments

Browsing History

Peter's Amazon.com

Today's Deals

Gift Cards & Registry

Sell

Help

EN

Hello, Peter

Account & Lists

Orders

Prime

Cart

Electronics > Accessories & Supplies > Audio & Video Accessories > Connectors & Adapters

You purchased this item on April 1, 2017.
View this order

uxcell

uxcell 6.7" x 3.1" Blue Metal Enclosure Project Case DIY Junction Box

★★★★☆ 6 customer reviews

Price: \$21.29 Prime

Only 6 left in stock - order soon.

Want it Wednesday, April 5? Order within 1 hr 19 mins and choose Two-Day Shipping at checkout. Details

Sold by uxcell and Fulfilled by Amazon. Gift-wrap available.

- Product Name : Junction Box; Mounted Type : Surface Mounted
- External Size : 170 x 130 x 80mm/6.7" x 5.1" x 3.1"(L*W*H); Internal Size : 160 x 120 x 70mm/ 6.3" x 4.7" x 2.7"(L*W*H)
- Material : Metal, Plastic; Color : Blue, White
- Net Weight : 450g
- Package : 1 x Junction Box

See more product details

New (2) from \$19.84 & FREE shipping.

Report incorrect product information.

Sling Television: 7 days FREE

Watch Live TV Programming Any Time and Anywhere. Simple monthly pricing, no long-term contracts or hidden fees. Watch now

Share

Qty: 1

Include 3-Year Protection Plan for \$4.97

Include 2-Year Protection Plan for \$3.10

Add to Cart

Turn on 1-Click ordering for this browser

Ship to:

Peter V. Radatti - Conshohocken - 19428

Add to List

Add to your Dash Buttons

Other Sellers on Amazon

Amazon.com AmazonBasics USB 3.0 Extension Cable – A-Male to A-Female 9.8 Feet \$6.49



This screenshot shows the Amazon.com product page for the AmazonBasics USB 3.0 Extension Cable – A-Male to A-Female - 9.8 Feet. The page features a large image of the black USB cable on the left. To the right, the product title is displayed in bold, followed by a star rating and the number of customer reviews. The price is listed as \$6.49, with a Prime logo indicating fast shipping. Below the price, there is a note about stock availability and a countdown timer for a tomorrow deal. The product details section lists specifications such as length, connector type, and material. On the right side of the page, there are options to add the item to the cart, a section for protection plans, and a shipping address field. The Amazon Prime logo and a search bar are visible at the top of the page.

amazon Prime

Electronics

Departments

Browsing History

Peter's Amazon.com

Today's Deals

Gift Cards & Registry

Sell

Help

EN

Hello, Peter

Account & Lists

Orders

Prime

Cart

Electronics > Computers & Accessories > Computer Accessories & Peripherals > Cables & Interconnects > USB Cables

You purchased this item on April 2, 2017.
Size: 9.8 Feet | Product Packaging: Frustration-Free Packaging | View this order

AmazonBasics

AmazonBasics USB 3.0 Extension Cable - A-Male to A-Female - 9.8 Feet (3.0 Meters)

★★★★☆ 2,018 customer reviews | 92 answered questions

Price: \$6.49 Prime | FREE One-Day

Delivered tomorrow for FREE with qualifying orders over \$35. Details

In Stock.

Get it tomorrow, April 4. Order within 17 hrs 19 mins and choose Same-Day Delivery at checkout. Details

Ships from and sold by Amazon.com in easy-to-open packaging. Gift-wrap available.

Size: 9.8 Feet

3 Feet/2-Pack 6 Feet/2-Pack 9.8 Feet

Product Packaging: Frustration-Free Packaging

Standard Packaging Frustration-Free Packaging

- One 9.8-foot-long (3 meters) USB 3.0 A-Male to A-Female high-speed extension cable
- Extends your USB connection to your computer by 9.8 feet; for use with printers, cameras, mice, keyboards and other USB computer peripherals
- Constructed with corrosion-resistant, gold-plated connectors for optimal signal clarity and shielding to minimize interference
- Features shielding that provides protection against noise from electromagnetic and radio-frequency signals, keeping your signal clear with less loss of bandwidth for higher performance
- USB 3.0 uses less power, but has increased power output – up to 4.8 Gb/s. Compared with the USB 2.0 transmission speed, USB 3.0 is 10 times faster

Share

Qty: 1

Add to Cart

Turn on 1-Click ordering for this browser

Ship to:

Peter V. Radatti - Conshohocken - 19428

Add to List

Add to your Dash Buttons

OR

Delivery available via Fresh

Get this item with your weekly groceries, delivered as quickly as same day or early next morning.

Have one to sell? Sell on Amazon

Amazon.com 10 Pack CESS Terminal Binding Post Power Audio Amp Plug Banana Jack \$6.79

amazon Prime

Electronics

Departments

Browsing History

Peter's Amazon.com

Today's Deals

Gift Cards & Registry

Sell

Help

Home Audio & Theater

Premium Audio

Headphones

Home Theater Systems

Speakers

Wireless Audio

Stereo System Components

Accessories

Deals

Electronics > Accessories & Supplies > Audio & Video Accessories > Connectors & Adapters

You purchased this item on March 18, 2017.
View this order

CESS
10 Pack CESS Terminal Binding Post Power Audio Amplifier Plug Banana Jack Socket 4511mm(LD)
★★★★☆ 5 customer reviews

Price: \$6.79 Prime

Only 14 left in stock - order soon.
Want it Wednesday, April 5? Order within 4 hrs 18 mins and choose Two-Day Shipping at checkout. Details
Sold by cessa4 and Fulfilled by Amazon. Gift-wrap available.

- Banana Plug Socket.
- Suitable for 4mm banana plugs.
- Diameter: 11mm L45mm
- Screw Bolt Diameter 2.75mm
- Color: Red and Black

New (1) from \$6.79 Prime

Report incorrect product information.

Sling Television: 7 days FREE
Watch Live TV Programming Any Time and Anywhere. Simple monthly pricing, no long-term contracts or hidden fees. Watch now

Share

Qty: 1

Add to Cart

Turn on 1-Click ordering for this browser

Ship to:
Peter V. Radatti - Conshohocken - 19428

Add to List

Add to your Dash Buttons

Have one to sell? Set on Amazon

belkin

Connect USB-C

Click to open expanded view

Amazon.com United Scientific WBP024-PK/6 Banana Plug Cord with Two-Way Stackable \$14.53

amazon Prime

Industrial & Scientific

Departments

Browsing History

Peter's Amazon.com

Today's Deals

Gift Cards & Registry

Sell

Help

Industrial & Scientific

Lab

Test & Measurement

Safety

Janitorial & Facilities

Food Service

Education

Material Handling

Materials

Metalworking

Electrical

Filtration

Deals

Instant Order Update for Peter V Radatti. You purchased this item on March 18, 2017. View this order.

Electronics > Portable Audio & Video > CB & Two-Way Radios > Accessories > Batteries

You purchased this item on March 18, 2017.
View this order

United Scientific Supplies
United Scientific WBP024-PK/6 Banana Plug Cord with Two-Way Stackable Banana Plugs at Both Ends, 24" Length, 3 Red and 3 Black (Pack of 6)
★★★★☆ 20 customer reviews

Was: \$19.24
Price: \$14.53 (\$2.42 / PACKAGE) Prime
You Save: \$4.71 (24%)

In Stock.
Want it Wednesday, April 5? Order within 4 hrs 18 mins and choose Two-Day Shipping at checkout. Details
Ships from and sold by Amazon.com.

Used & new (4) from \$13.06 Prime

Specifications for this item

Brand Name	United Scientific Supplies
Color	Red/Black
Item Weight	3 pounds
Length	24 inches
Model Number	WBP024-PK/6
Number of Items	6

Share

Qty: 1

Add to Cart

Turn on 1-Click ordering for this browser

Ship to:
Peter V. Radatti - Conshohocken - 19428

Add to List


Other Sellers on Amazon

\$14.53 (\$2.42 / PACKAGE) Prime
Sold by: Scientific Systems

\$15.95 (\$2.66 / PACKAGE)
Add to Cart


Conshohocken Radionics .

If you live near Southeastern Pennsylvania, you might wish to join. Membership and meetings are free. Their website is: <http://www.meetup.com/radionics/>

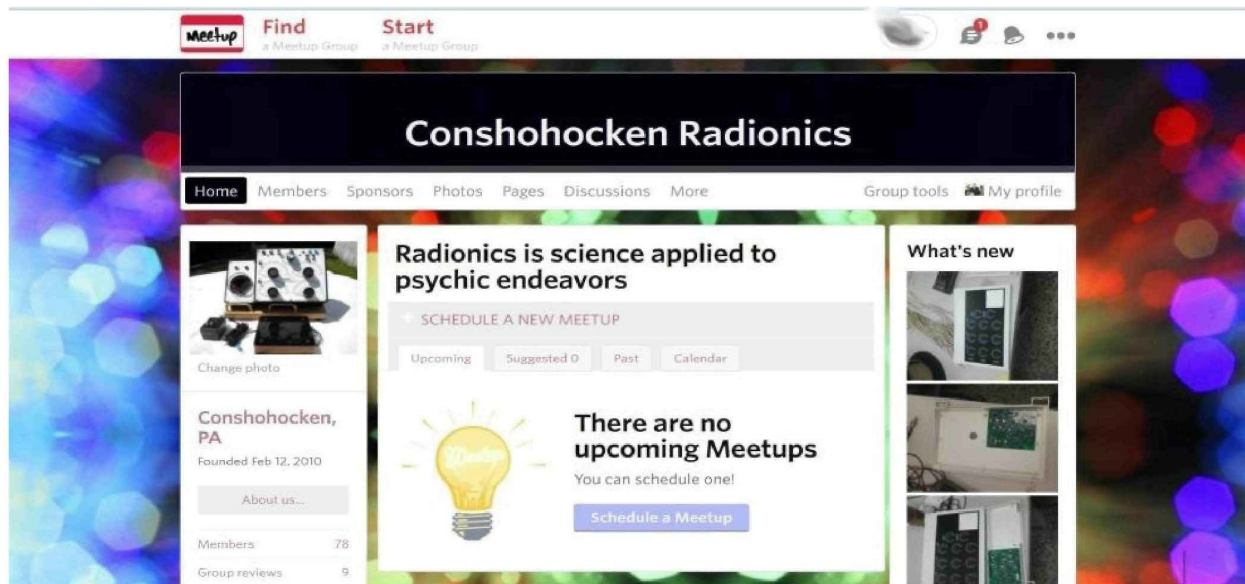


Dan Tuck's Manufacturer of Parcel Designed Thea Lamp and other useful devices.

<http://www.dtlightworks.com>

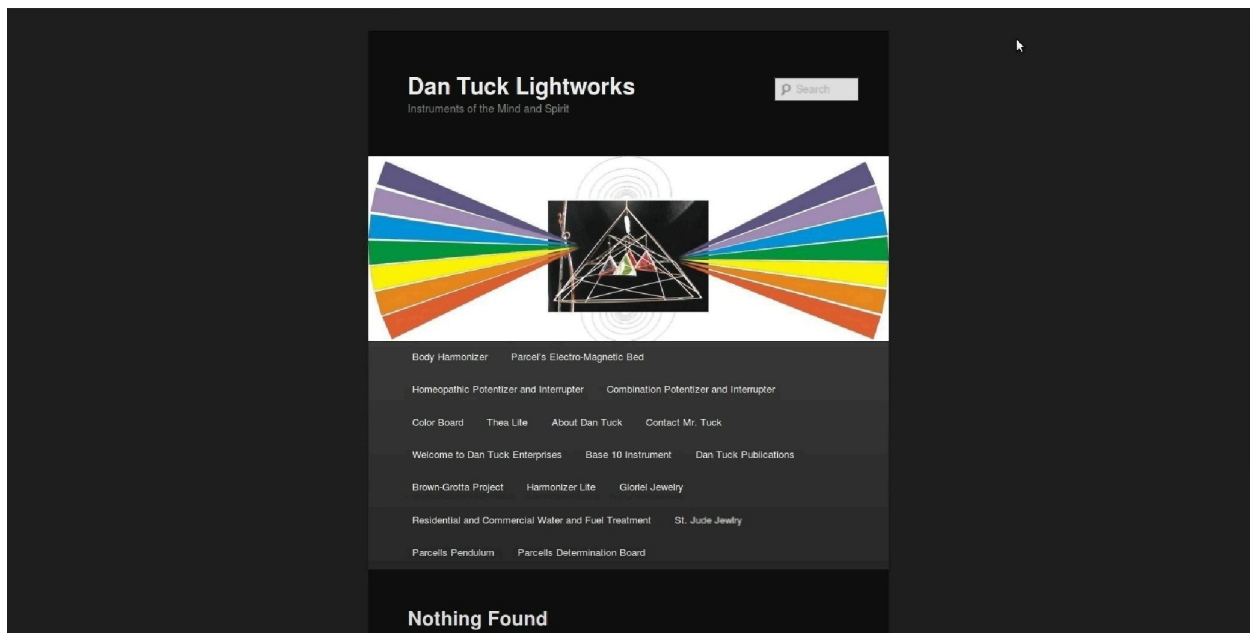

Chapter 8 - Bonus Material

If you want to integrate a computer into the E-Well so you don't have to carry it around or if you want to make your E-Well accessible over the Internet there is a cost effective and simple way of doing this. Use a Raspberry-Pi computer. These are \$35 and more powerful than is needed for this project. The only drawback is that you need to know how to configure the system for your purposes. The Raspberry uses Linux as the operating system. See photo below of a Raspberry Pi 2 Model B. (Image courtesy of pixabay.com) This computer contains 4 USB ports, a mini-usb port for power, HDMI and a RJ45 NIC. They can easily be added to a WiFi network.

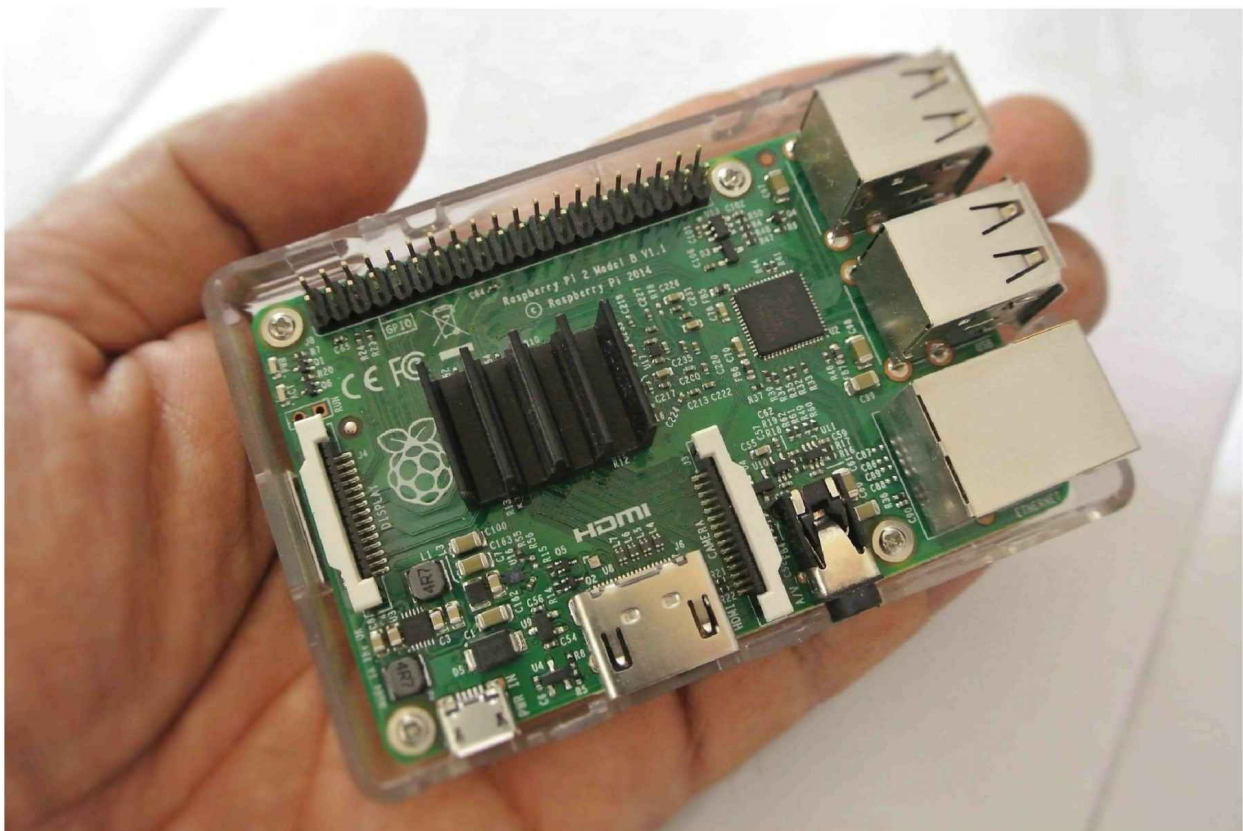

*End of Book
but not of your fun in Radionics!*

The Devil gave us Insomnia; God gave us Coffee! - Pete Radatti